
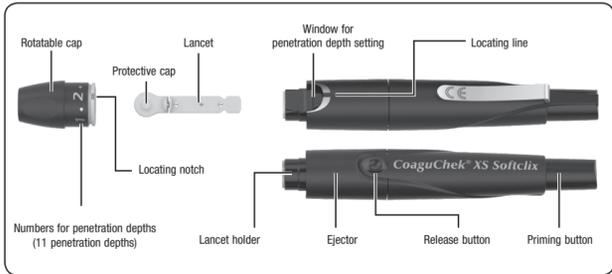













CoaguChek® XS Softclix

Lancing device and lancets Autopiqueur et lancettes



EN Instructions for Use

Intended Use

Lancing Device

The CoaguChek® XS Softclix lancing device is a device for simple, virtually pain-free collection of capillary blood from the fingertips. The CoaguChek® XS Softclix lancing device is intended for single patient use only! It is only allowed to be used to obtain blood from one person.

There is a risk of infections being transmitted if the lancing device is used by other people, even by family members, or if healthcare professionals use this lancing device to obtain blood from different people. This lancing device is therefore not suitable for professional use in healthcare facilities and institutions. It is not a sterile product.

People in the area of coagulation self-monitoring are considered as target group.

Lancet

The CoaguChek® Softclix lancet is a sterile single-lancet and is intended to be used with the CoaguChek® XS Softclix lancing device for simple, virtually pain-free collection of capillary blood. The lancet is a disposable article intended to be used only once each.

Each lancet has a protective cap that guarantees sterile condition until its first use.

Before You Get Started

Read these instructions for use before you obtain a blood drop from your fingertip.

Information describing a situation for which there is a foreseeable serious hazard with the use of the device, is preceded by the following heading:

WARNING

Information regarding any special care you should exercise for the safe and effective use of the device, or to avoid damage to the device that could occur as a result of use, including misuse, is preceded by the following heading:

PRECAUTION

Precautions and Warnings

WARNING

Risk of suffocation

This product contains small parts that can be swallowed. Keep this product away from people who might swallow it, for example, small children.

Risk of infection

During obtaining a blood drop, the lancing device may come into contact with blood.

To prevent infections from being transmitted, the lancing device must not be used by other people, even by family members. Healthcare professionals must not use the lancing device to obtain blood from different people.

Risk of infection

The lancing device or lancet has come into contact with blood and has protruding sharps due to damage.

To prevent infections from being transmitted, check the lancing device and lancet for damages. Dispose of a damaged lancing device as infectious material according to the regulations applicable in your country. Dispose of a damaged lancet in such a way as to prevent injury from the needles. For example, place the lancet into a cannula disposal container.

PRECAUTION


Risk of infection

The lancing device or lancet has come into contact with blood and has protruding sharps due to damage.

PRECAUTION

Risk of infection

The lancing device or lancet has come into contact with blood and has protruding sharps due to damage.

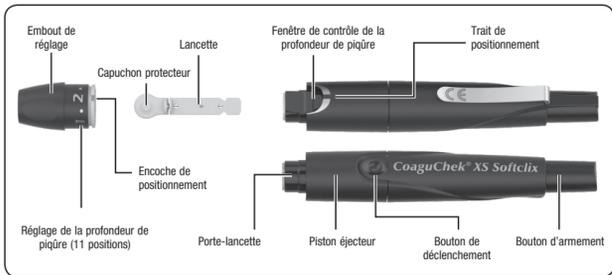

FR Instructions d'utilisation

Utilisation prévue

Autopiqueur

L'autopiqueur CoaguChek® XS Softclix permet de prélever facilement et pratiquement sans douleur du sang capillaire sur l'extrémité du doigt. L'autopiqueur CoaguChek® XS Softclix est réservé exclusivement à l'usage personnel ! Il doit uniquement servir au prélèvement de sang chez une seule personne.

Il existe un risque de transmission d'infections si l'autopiqueur est utilisé par d'autres personnes, notamment les membres d'une même famille, ou si les professionnels de la santé emploient l'autopiqueur pour prélever le sang de plusieurs personnes. Cet autopiqueur ne convient donc pas à un usage professionnel en établissement hospitalier. Ce produit n'est pas stérile.

Les personnes travaillant dans le domaine de l'autocntrôle de la coagulation sont considérées comme un groupe cible.

Lancette

La lancette CoaguChek® Softclix est une lancette à usage unique stérile conçue pour être utilisée avec l'autopiqueur CoaguChek® XS Softclix et qui permet de prélever facilement et pratiquement sans douleur du sang capillaire sur l'extrémité du doigt. La lancette est un article jetable destiné à n'être utilisé qu'une fois.

Chaque lancette présente un capuchon protecteur garantissant sa stérilité jusqu'à la première utilisation.

Avant de commencer

Lisez ces instructions d'utilisation avant de prélever une goutte de sang de l'extrémité de votre doigt.

Les informations décrivant une situation présentant un danger grave prévisible avec l'utilisation de ce dispositif sont précédées du libellé suivant :

AVERTISSEMENT

Les informations sur les précautions particulières à prendre pour une utilisation sûre et efficace du dispositif, ou pour éviter un endommagement du dispositif en raison de l'utilisation, y compris une mauvaise utilisation, sont précédées du libellé suivant :

PRECAUTION

Précautions et avertissements

AVERTISSEMENT

Risque d'étouffement

Ce produit contient de petites pièces pouvant être ingérées. Conservez ce produit hors de portée des personnes pouvant les avaler, comme les jeunes enfants.

Risque d'infection

Pendant le prélèvement d'une goutte de sang, l'autopiqueur peut entrer en contact avec le sang.

Afin de prévenir la transmission d'infections, l'autopiqueur ne doit pas être utilisé par d'autres personnes, même les membres de la famille. Les professionnels de santé ne doivent pas utiliser l'autopiqueur pour prélever du sang chez d'autres personnes.

Risque d'infection

L'autopiqueur ou la lancette est entrée en contact avec du sang et présente des parties tranchantes saillantes en raison de dommages.

Afin de prévenir la transmission d'infections, contrôlez l'absence de dommages sur l'autopiqueur et les lancettes. Éliminez un autopiqueur endommagé avec les matériaux infectieux conformément à la réglementation en vigueur dans votre pays. Éliminez une lancette endommagée de manière à éviter toute blessure due aux aiguilles. Par exemple, placez la lancette dans un récipient pour l'élimination des canules.

PRECAUTION

Risk of injury

Skin contact to the lancing device or lancet may cause skin irritation.

If your skin becomes irritated or inflamed, consult your healthcare professional.

Risk of injury

The needle of the lancet is damaged due to use on a hard surface.

Only use the lancet to obtain a blood drop.

Risk of injury

Parts of the lancing device, for example, the priming button, may shoot away during use.

Do not point the lancing device at your face or other people.

If the lancing device or lancet was dropped or exposed to other mechanical stress, check them for damages, for example, cracks. Do not use them if they are damaged.

Only insert CoaguChek® Softclix lancets into the CoaguChek® Softclix lancing device. Other lancets may impair the operation of the lancing device or damage it permanently.

Preparation

► Wash your hands with warm water and soap before you obtain blood (see ➊). Dry your hands thoroughly. This reduces contamination of the puncture site and stimulates blood flow.

Inserting the Lancet

You have to insert a lancet to be able to obtain blood with the lancing device.

WARNING

Risk of infection

If the protective cap is damaged or missing, the needle can be unsterile and lead to infection.

Visually inspect the lancet. If the protective cap is deformed, cracked, or otherwise damaged, do not use the lancet. If the protective cap is missing or any part of the needle is exposed, do not use the lancet. Discard the lancet.

► Remove the cap from the lancing device (see ➊).

► Insert a new lancet into the lancet holder as far as it will go (see ➋).

You must hear the lancet click into place.

► Twist the protective cap off of the lancet (see ➌).

► Place the cap back on again.

The locating notch in the cap must be directly aligned with the locating line on the lancing device (see ➍). You must hear the cap click into place.

Setting the Penetration Depth

You can set 11 penetration depths (0.5 to 5.5), so that you can adjust the penetration depth to the texture of your skin. The penetration depth set is shown in the window. The larger the number, the greater the penetration depth.

If you have no experience with this lancing device, we recommend setting a low penetration depth, such as penetration depth 2.

► Rotate the cap until the desired penetration depth is displayed in the window (see ➎).

WARNING

Risk of injury

If the penetration depth is too large, the puncture can injure children.

Before using the lancing device for the first time on children, ask your healthcare professional. Start with the lowest penetration depth.

Priming the Lancing Device

In order to be able to obtain blood, you must prime the lancing device. Only prime the lancing device just before obtaining blood.

► Press the priming button down as far as it will go (see ➏). Do not press the release button simultaneously.

The lancing device is primed when the centre of the release button is yellow (see ➐).

Obtaining a Blood Drop

WARNING

Risk of infection

The lancet was used several times to obtain blood.

To prevent infections from being transmitted, use the lancet only once to obtain blood.

Risk of infection

In rare cases, the lancet is not pulled back into the lancing device after you obtained blood.

To prevent infections from being transmitted, check that the lancet does not protrude from the cap after you obtained blood. If the lancet protrudes, do not touch the front of the cap. Remove the cap from the lancing device with care. Eject the lancet and dispose of it. Dispose of used lancets in such a way as to prevent injury from the needles. For example, place the lancet into a cannula disposal container.

PRECAUTION

Risk of infection

The puncture site was not cleaned.

Before obtaining blood clean the puncture site.

Risk of infection

The use by date of the lancet has expired.

Use only lancets that are within the use by date. The use by date is printed next to the μ symbol on the packaging.

In general, blood can be obtained from any finger. Certain fingers can be unsuitable if, for example, a skin or fingernail infection is present. We recommend obtaining capillary blood from the sides of the fingertips as these areas are the least sensitive to pain. Use a new lancet each time you obtain blood so that obtained blood remains virtually pain free.

Only use the lancing device when the cap is attached. Without the cap, the lancet penetrates too deeply and the puncture can become painful.

► Press the lancing device firmly against the selected puncture site (see ➑).

► Press the release button (see ➑).

The lancet is released and it penetrates the skin.

► Massage the finger in the direction of the fingertip to encourage a blood drop to form.

The amount of blood that emerges depends on the penetration depth and the pressure used to hold the lancing device against the skin.

If not enough blood emerges, apply more pressure on the lancing device when you next obtain blood. If that is not sufficient, increase the penetration depth progressively in addition.

If too much blood emerges, decrease the penetration depth.

► Test your coagulation value immediately after you obtained blood, according to the instructions for use for your CoaguChek instrument.

We recommend protecting the puncture site from contamination afterwards.

Ejecting the Used Lancet

► Remove the cap from the lancing device (see ➊).

► Slide the ejector forward (see ➑).

The used lancet is ejected.

► Place the cap back on again.

► Dispose of used lancets according to local regulations.

Precaution

Risk of infection

The needle of a used lancet is not protected and can be touched accidentally.

To prevent infections from being transmitted, dispose of used lancets in such a way as to prevent injury from the needles. Place the lancet, for example, into a cannula disposal container.

Réglage de la profondeur de piqûre

Vous pouvez régler 11 profondeurs de piqûre (de 0.5 à 5.5) afin d'ajuster la profondeur de piqûre en fonction de la texture de votre peau. La profondeur de piqûre définie est affichée dans la fenêtre de contrôle. Plus le numéro est haut, plus la piqûre est profonde.

Si vous n'avez pas l'habitude de manipuler l'autopiqueur, il est conseillé d'essayer tout d'abord une faible profondeur de piqûre, la position 2 par exemple.

► Tournez l'embout jusqu'à atteindre la profondeur de piqûre souhaitée (voir ➎).

AVERTISSEMENT

Risque de blessure

Si la profondeur de piqûre est trop importante, la piqûre peut blesser les enfants.

Avant d'utiliser l'autopiqueur pour la première fois sur un enfant, demandez conseil à votre professionnel de santé. Commencez par la profondeur de piqûre la plus faible.

Armement de l'autopiqueur

Afin de pouvoir prélever du sang, vous devez armer l'autopiqueur. Armez l'autopiqueur seulement juste avant de prélever du sang.

► Appuyez sur le bouton d'armement jusqu'à la butée (voir ➏). Veillez à ne pas appuyer en même temps sur le bouton de déclenchement.

L'autopiqueur est armé lorsqu'une surface jaune apparaît au centre du bouton de déclenchement (voir ➐).

Prélèvement d'une goutte de sang

AVERTISSEMENT

Risque d'infection

La lancette a été utilisée plusieurs fois pour prélever du sang.

Afin de prévenir la transmission d'infections, utilisez la lancette pour un seul prélèvement de sang.

Risque d'infection

Dans de rares cas, la lancette n'est pas réinsérée dans l'autopiqueur après le prélèvement de sang.

Afin de prévenir la transmission d'infections, vérifiez que la lancette ne dépasse pas de l'embout après le prélèvement de sang. Si la lancette dépasse, ne touchez pas l'avant de l'embout. Retirez l'embout de l'autopiqueur avec précaution. Éjectez la lancette et éliminez-la. Éliminez les lancettes usagées de manière à éviter toute blessure due aux aiguilles. Par exemple, placez la lancette dans un récipient pour l'élimination des canules.

Éjection de la lancette usagée

► Retirez l'embout de l'autopiqueur (voir ➊).

► Faites glisser le piston éjecteur vers l'avant (voir ➑). La lancette usagée est éjectée.

► Remplacez l'embout.

► Éliminez les lancettes usagées conformément à la réglementation locale en vigueur.

Operating Conditions

Use the lancing device including accessories under the following operating conditions:

- Temperature range: +5 to +45 °C
- Relative humidity range: 5 to 90 %

Storing the Lancing Device and Lancets

Do not store the lancing device in a primed state. Do not store the lancing device and lancets at extreme temperatures, for example, in a hot car. This can impair the operation of the lancing device and lancets.

Store the lancing device only without a lancet inserted.

Cleaning and Disinfecting the Lancing Device and Cap

PRECAUTION

Risk of infection

The lancing device and cap may have come into contact with blood.

To prevent infections from being transmitted, clean and disinfect the lancing device and cap always before someone else handles them, for example, to assist you.

To prevent infections from being transmitted, you must clean and disinfect the lancing device and cap regularly:

- At least once a week
- When there is blood on the lancing device or cap
- Always before someone else handles the lancing device, for example, to assist you.

You need lint-free cloths in which you can wrap the whole lancing device, water and 70 % isopropanol.

Before you disinfect the lancing device and the cap, you first have to clean them to remove blood and other dirt.

To avoid damaging the lancing device and the cap:

- Do not dip the lancing device and the cap in the fluids.
- Use only water for cleaning and only 70 % isopropanol for disinfecting.

► Remove the cap from the lancing device (see ➊).

► Eject the lancet (see ➑).

► Moisten a cloth with water.

► Wipe the lancing device and the cap thoroughly. Wipe the lancing device from the outside only (see ➒) and the cap from the outside and the inside (see ➓).

► Dry the lancing device and the cap with a dry cloth.

Disinfecting

► Dampen a cloth with 70 % isopropanol.

► Wipe the lancing device and the cap thoroughly for 2 minutes each. Wipe the lancing device from the outside only and the cap from the outside and the inside.

► Place the cap back on again.

► Wrap the whole lancing device in the cloth.

► Leave the lancing device wrapped for 8 minutes.

► Unwrap the lancing device and let it dry in the air.

Disposing of the Lancing Device

PRECAUTION

Risk of infection

The lancing device has come into contact with blood and is disposed of improperly.

To prevent infections from being transmitted, dispose of the used lancing device as infectious material according to the regulations applicable in your country.

During obtaining a blood drop, the lancing device may come into contact with blood. A used lancing device therefore carries a risk of infection.

Dispose of an unused lancing device as plastic waste.

For information about correct disposal, contact your local council or authority.

Ordering Information

If you want to order a CoaguChek® XS Softclix lancing device or CoaguChek® Softclix lancets, contact customer support.

Additionally-required Materials

CoaguChek® Softclix lancets, 50 lancets, REF 03506509001.

Reporting of Serious Incidents

For a patient/user/third party in the European Union and in countries with identical regulatory regime (Regulation 2017/745/EU on medical devices); if, during the use of this device or as a result of its use, a serious incident has occurred, please report it to the manufacturer and to your national authority.



Last Update

</

CoaguChek® XS Softclix

Nakuwacz i lancety

Sprožilna naprava in lancete

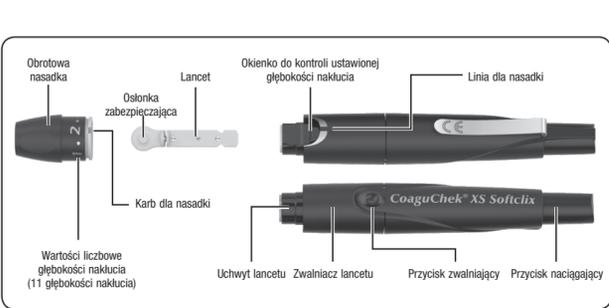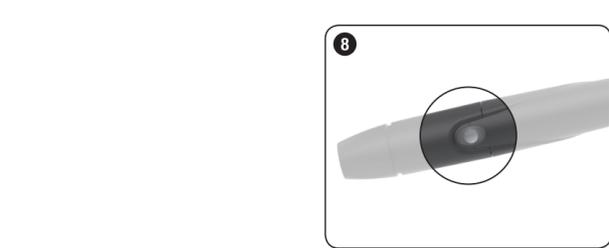

Instrukcija obsługi

Zastosowanie
Nakuwacz Nakuwacz CoaguChek® XS Softclix jest urządzeniem do łatwego, prawie bezbolesnego pozyskiwania krwi kapilarnej z opuszki palca. Nakuwacz CoaguChek® XS Softclix jest przeznaczony wyłącznie do użyciu przez jednego pacjenta! Wolno nim pozyskiwać krew zawsze tylko od tej samej osoby.

Stosowanie nakuwacza przez inne osoby, również członków rodziny, lub wykorzystywanie go przez personel medyczny do pozyskiwania krwi u różnych pacjentów grozi niebezpieczeństwem przeniesienia zakażeń. Z tego powodu nakuwacz ten nie jest przeznaczony do profesjonalnego stosowania w placówkach służby zdrowia. Nie jest to produkt sterylny.

Za grupę docelową uważa się osoby samodzielnie kontrolujące krzepliwość krwi.

Lancet


Lancet CoaguChek® Softclix to sterylny lancet jednorazowego użytku przeznaczony do stosowania z nakuwaczem CoaguChek® XS Softclix w celu prostego, praktycznie bezbolesnego pobierania krwi kapilarnej. Lancet jest artykułem jednorazowego użytku, czyli przeznaczonym do zastosowania tylko jeden raz.

Każdy lancet posiada osłonkę zabezpieczającą, która gwarantuje sterylność do pierwszego użycia.

Przed rozpoczęciem stosowania

Przed pozyskaniem kropli krwi z opuszki palca należy przeczytać niniejszą instrukcję obsługi.

Informacje opisujące sytuację, w której istnieje przewidywalne poważne zagrożenie związane z użytkowaniem wyrobu, są poprzedzone następującym nagłówkiem:

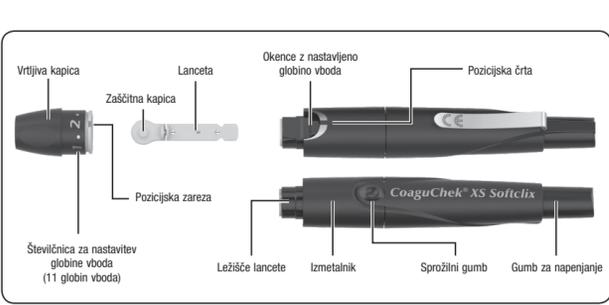

Navodila za uporabo

Predvidena uporaba
Sprožilna naprava Sprožilna naprava CoaguChek® XS Softclix je naprava za preprosto, skoraj neboleče odvzemanje kapilarne krvi na prstnih blazincah. Sprožilna naprava CoaguChek® XS Softclix je predvidena za uporabo na samo enem bolniku! Za odvzem krvi jo je dovoljeno uporabiti samo pri eni osebi.

Če sprožilno napravo uporabljajo drugi ljudje, tudi družinski člani, ali če zdravstveni delavci uporabljajo to sprožilno napravo za odvzem krvi pri različnih ljudeh, obstaja nevarnost prenosa okužb. Sprožilna naprava zato ni primerna za profesionalno uporabo v zdravstvenih ustanovah in institucijah. Izdelek ni sterilen.

Ciljna skupina so ljudje na področju samoopazovanja koagulacije.

Lanceta
































































































Lanceta CoaguChek® Softclix je sterilna lanceta za enkratno uporabo in je namenjena za uporabo s sprožilno napravo CoaguChek® XS Softclix za enostavno, skoraj neboleče odvzemanje kapilarne krvi. Lanceta je izdelek, ki je primeren za enkratno uporabo.

Vsaka lanceta ima zaščitno kapico, ki zagotavlja sterilno stanje do prve uporabe.

Preden začnete

Preden odvzimate kapiljno krvi na prstni blazinic, preberite ta navodila za uporabo.

Prad podatki, ki opisujejo položaj, v katerem obstaja predvidljiva resna nevarnost na podlagi uporabe naprave, je navedeno naslednje besedilo:



ŚRODEK OSTROŻNOŚCI

Możliwość zranienia się
Kontakt skóry z nakuwaczem lub lancetem może spowodować podrażnienie skóry.

Jeśli skóra ulegnie podrażnieniu lub wystąpi stan zapalny, skonsultuj się z przedstawicielem służby zdrowia.

Możliwość zranienia się
Ostrze lanceta jest uszkodzone w wyniku użycia go na twardej powierzchni.

Lancetu należy używać wyłącznie do pozyskania kropli krwi.

Możliwość zranienia się
Części nakuwacza, np. przycisk naciągający, mogą odstrzelić podczas użytkowania.

Nie należy kierować nakuwacza w stronę twarzy lub innych osób.

Jeżeli nakuwacz lub lancet został upuszczony lub był narażony na działanie innych sił mechanicznych, należy sprawdzić, czy wyrób nie jest uszkodzony, np. pełnięty. Nie należy używać wyrobów, jeśli zostały uszkodzone.

W nakuwacza CoaguChek® Softclix stosuj wyłącznie lancety CoaguChek® Softclix. Inne lancety mogą doprowadzić do nieprawidłowego działania nakuwacza lub zniszczyć nakuwacz.

Przygotowania
▶ Przed pozyskaniem krwi umyć dłonie ciepłą wodą i mydłem (patrz ➊). Dłonie należy dobrze wysuszyć. Zapobiegnie to zabrudzeniu miejsca wkucia i poprawi przepływ krwi.

Włożenie lancetu
Aby wykorzystać nakuwacza do pozyskania krwi należy najpierw włożyć lancet.

OSTRZEŻENIE
Ryzyko uduszenia
Produkt zawiera niewielkie elementy, które mogą zostać połknięte.

Wyrób należy przechowywać poza zasięgiem osób, które mogą go połknąć, np. małych dzieci.

Ryzyko zakażenia
Podczas pobierania kropli krwi może dojść do kontaktu nakuwacza z krwią.

Aby zapobiec przenieszeniu zakażeń, z nakuwacza nie mogą korzystać inne osoby, nawet jeśli są to członkowie rodziny. Pracownikom służby zdrowia nie wolno używać nakuwacza do pobierania krwi od różnych osób.

Ryzyko zakażenia
Nakuwacz lub lancet wszedł w kontakt z krwią i ma wystające ostre krawędzie z powodu uszkodzenia.

Aby zapobiec przeniesieniu zakażeń, należy sprawdzić, czy nakuwacz i lancet nie są uszkodzone. Usunąć zużyty nakuwacz, jako materiał potencjalnie zakaźny zgodnie z przepisami obowiązującymi w danym kraju. Usuwać uszkodzone lancety tak, aby wykluczone było skałeczenie się o ostrza lancetów. Na przykład, umieścić lancet w pojemniku na zużyte kaniule.

PREVIDNOSTNI UKREP
Tveganje za poškodbo
Stik kože s sprožilno napravo ali lanceto lahko draži kožo. Če se koža razdrži ali vname, se posvetujte s svojim zdravstvenim delavcem.

Tveganje za poškodbo
Igla lancete je poškodovana zaradi uporabe na trdi površini.

Lanceto uporabite le za odvzem kapiljne krvi.

Tveganje za poškodbo
Deli sprožilne naprave, na primer gumb za napenjanje, se lahko med uporabo odbijejo.

Sprožilne naprave ne usmerjajte v obraz ali druge ljudi.

Če sprožilna naprava ali lanceta pade ali pa je izpostavljena drugim mehanskim obremenitvam, prevrte, ali so vidne poškodbe, na primer razpoke, Če sta izdelka poškodovana, ju ne uporabljajte.

V sprožilno napravo CoaguChek® Softclix vstavite izključno lancete CoaguChek® Softclix. Druge lancete lahko poslabšajo delovanje sprožilne naprave ali pa jo trajno poškodujejo.

Priprava
▶ Pred odvzemanj krvi si umijte roki s toplo vodo in z milom (glejte ➊). Temeljito si posušite roke. To zmanjša kontaminacijo mesta vboda in spodbudi pretok krvi.

Vstavljanje lancete
Za odvzem krvi s sprožilno napravo morate vstaviti lanceto.